



Combustion Analyzer

for Commercial & Light Industrial Use



Combustion & Emissions

P/N: 0024-9553 | January 2018 Revision 1

Quick Start Guide



For more detailed product information, scan here or visit www.mybacharach.com to access the PCA® 400 User Manual (P/N 0024-9551).

1. Introduction

The PCA® 400 is a commercial grade, hand-held combustion and emissions analyzer for on-demand or semi-continuous sampling of light industrial, institutional, commercial, and residential furnaces, boilers, and appliances. The base instrument is supplied with a probe and hose assembly, factory calibrated and installed sensors, printer interface, hard carry case, filters, USB cable, PC Software, AC adapter, and rechargeable lithium-ion battery pack. The reporting kit version includes (in addition to the base configuration) a Bluetooth® + IrDA printer.

2. Safety Instructions

CODE COMPLIANCE: Comply with all local and national laws, rules and regulations associated with this equipment. Operators should be aware of the regulations and standards in their industry / country for the operation of this analyzer.




WARNING: This analyzer is not intended to be used as a safety device.



WARNING: This analyzer has not been designed to be intrinsically safe for use in areas classified as hazardous locations.


3. Component Overview

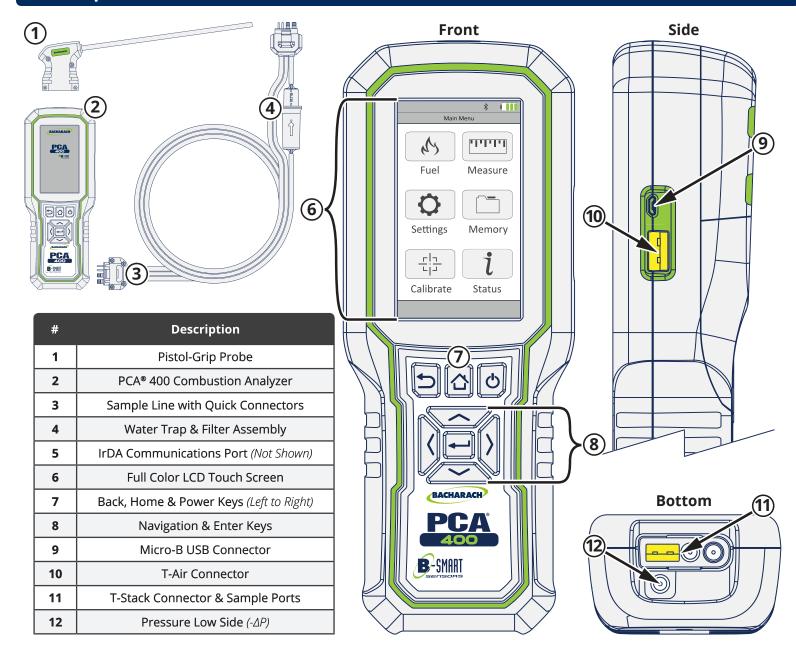

4. Prerequisites



IMPORTANT: Ensure that the water trap assembly is clean, dry, and properly assembled.






IMPORTANT: Check for obvious signs of splits and / or cracks in the tubing.




IMPORTANT: Perform routine maintenance (replacing sensors, calibrating, etc.) as outlined in the PCA® 400 User Manual (P/N 0024-9551).





IMPORTANT: Ensure that the analyzer has sufficient charge before operation. If in doubt, recharge lithium-ion battery, replace disposable batteries, or provide power via the AC adapter and USB cable.

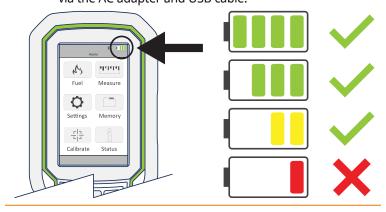



5. Hardware Setup

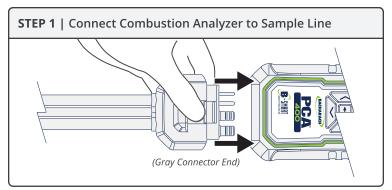

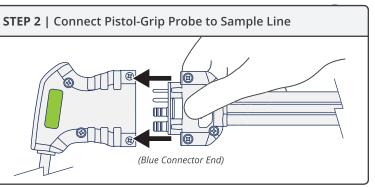

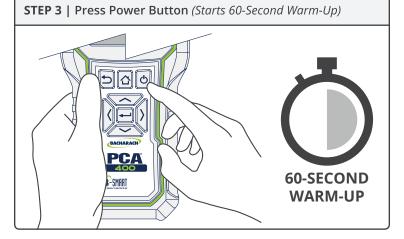








Bacharach, Inc. 621 Hunt Valley Circle, New Kensington, PA 15068 USA

Bacharach USA Customer Service: +1 724 334 5000 Bacharach CAN Customer Service: +1 905 470 8985 mybacharach.com | help@mybacharach.com


6. Operation Overview

STEP 1 | Select Fuel Type

Access the Fuel Menu (إح) from the Main Menu and select the type of fuel used in the application being measured.

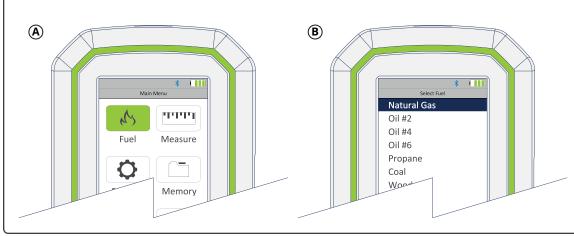


Warning: When testing an appliance, a full visual inspection should be performed to ensure its safe operation.

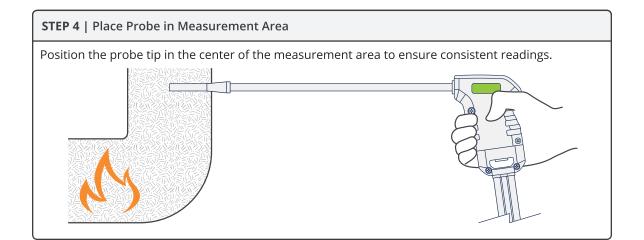


STEP 2 | Configure Memory (Optional)

Access the Memory Menu (()) and select the folder / memory location where data will be saved; touch folder / memory location to access memory configuration screen. (If no location is selected, analysis results will be saved to the "Default" folder.)

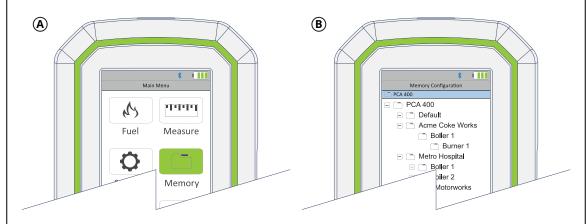

STEP 3 | Select Measurement Type

Access the Measure Menu (m) from the Main Menu and select the type of test which you will be performing.

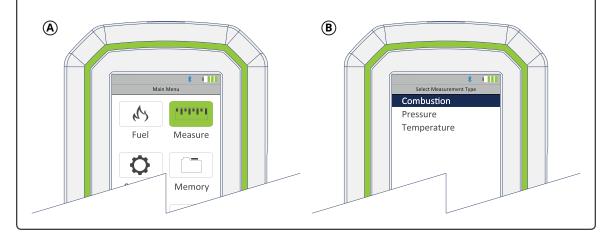

STEP 5 | Perform Combustion Analysis

Press the Start Icon (▶) to start the pump and begin analysis. After the results have stabilized, press the Pause Icon (II) to stop the pump. (The status of the pump is indicated at the top of the analyzer screen: ⑤ indicates that the pump is on, ② indicates that the pump is off.)



STEP 6 | Save & Print Results of Combustion Analysis

After stopping the pump, press the Save Icon () to save the data to the folder / memory location configured in step 2. After saving the data, press the Print Icon () to print the test results using a connected IrDA + Bluetooth Printer. (The data display can be toggled between several display options by pressing).











7. Post-Analysis Maintenance



CAUTION: The probe may be hot after analysis and can cause bodily harm and or damage the analyzer. Allow the probe sufficient time to cool before handling or storing in the supplied instrument case.

The probe and sample line may become dirty during normal use and should be cleaned regularly to ensure proper function. The following maintenance should be performed after each use:

- \square Allow the analyzer to purge in fresh air for a minimum of 10-minutes or until O_2 is greater than 20% & other measured readings are less than 5ppm.
- Remove excess moisture from Water Trap, Sample Line and Pistol-Grip Probe.
- Clean debris from probe and analyzer.
- ☐ Charge analyzer batteries before storage.

8. Parts & Accessories



IMPORTANT: Use only original equipment components with this device.



CAUTION: Except for sensor and battery replacement, this analyzer should only be opened and / or serviced by authorized Bacharach personnel. Failure to comply may void the warranty.

| Product | Desc | ription / Part Number |
|---------------------------|--------------|---|
| | Description: | The Sample Conditioner extracts water vapor from samples, allowing the PCA® 400 to accurately read levels of NO ₂ and or SO ₂ . |
| Sample Conditioner | P/N: | 0024-7400 |
| | Description: | 7.5' Viton® Sample Line with quick connectors allows the PCA® 400 to accurately read levels of NO_2 and or SO_2 . |
| Viton® Sample Line | P/N: | 0024-3236 |
| IrDA + Bluetooth® | Description: | The IrDA + Bluetooth® Printer allows technicians to print reports directly from the PCA® 400 without a wired connection. |
| Printer | P/N: | 0024-1680 |
| Printer Paper | P/N | 0024-1310 (contains 5 rolls of paper) |
| Water Trap Filters | P/N | 0007-1644 (contains 3 filters) |
| O ₂ Sensor | P/N | 0024-1652 |
| CO _{Low} Sensor | P/N | 0024-1687 |
| CO _{HIGH} Sensor | P/N | 0024-1542 |
| SO₂ Sensor | P/N | 0024-1543 |
| NO₂ Sensor | P/N | 0024-1544 |
| NO Sensor | P/N | 0024-1691 |